



## DRILLING FLUIDS EQUIPMENT

For over 30 years OFI Testing Equipment (OFITE) has provided instruments and reagents for testing drilling fluids, well cements, completion fluids, and wastewater. In addition to these product lines we also offer a range of instruments for core analysis. From our manufacturing facility in Houston, TX we provide customers all over the world with quality products and exceptional service.

Our drilling fluids product line includes innovative designs such as the Model 900 Viscometer, which showcases our ability to develop new technology to meet customer and industry demands. We also offer Retorts, Aging Cells, Roller Ovens, Mud Balances, Filter Presses, and all other instruments required to evaluate drilling fluid properties according to API Recommended Practice 13B-1 and 13B-2.

As an independent manufacturer and supplier, OFITE has one priority, our customers.

### OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Dr.

Houston, TX 77065

877.837.8683

[www.ofite.com](http://www.ofite.com)

©Copyright OFITE 2015



## Mud Balance, 4 Scale, Plastic

The plastic mud balance is engineered so that the mud cup at one end of the beam is balanced by a fixed counterweight at the other end, with a sliding-weight rider that moves along a graduated scale. A level bubble is mounted on the beam to ensure accurate balancing.



## Features


- Plastic will not corrode when using corrosive fluids
- Full size, full scale mud balance
- Two most popular scales are on top for easy reading
- Can be easily cleaned
- Accurate density analysis

## Technical Specifications and Requirements

- 100-00 - Mud Balance, 4 Scale, Plastic

### Specifications

- Density Ranges
  - 8.0 - 25.0 lb / gal
  - 960 - 3000 Specific Gravity, kg/meter<sup>3</sup>
  - 60 - 189 lb / ft<sup>3</sup>
  - 420 - 1300 pounds per inch<sup>2</sup> / 1000 ft
- Size: 21.5" × 5" × 4.5" (55 × 13 × 11 cm)
- Weight: 3 lb (1.4 kg)

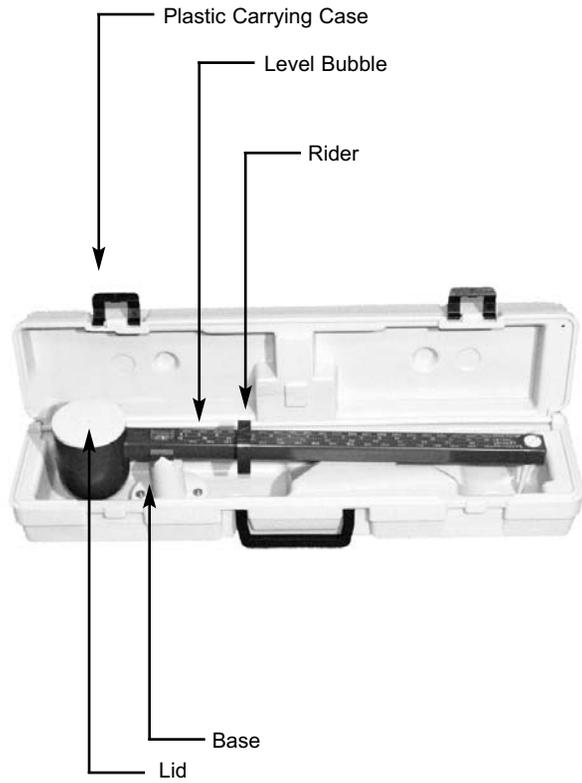

**4-Scale Plastic Mud Balance  
Complete with Case  
100-00**

**Components:**

**#100-01 4-Scale Plastic Mud Balance w/o Case**


- #100-10 Base
- #100-20 Lid
- #100-25 Rider
- #100-30 Level Bubble Assembly**
  - #100-28 Level Bubble Frame
  - #100-29 Level Bubble Vial
- #100-56 Lead Shot

**Case:**

- #100-40 Plastic Carrying Case

**OFI Testing Equipment, Inc.**  
 11302 Steeplecrest Dr. Houston, Texas 77065 U.S.A.  
 Tele: 832.320.7300 or 877.837.8683  
 Fax: 713.880.9886 [www.ofite.com](http://www.ofite.com)

©Copyright OFITE 2011

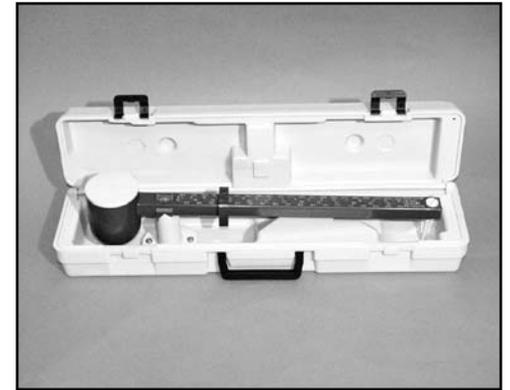

**4-Scale Plastic Mud Balance**

**Item# 100-00**

**Instruction Manual**

**Updated 4/21/2009  
Ver. 1.2**

**OFI Testing Equipment, Inc.**

**Introduction:**

The density or weight of a given volume of liquid is determined by using a mud balance. The arm is graduated and permits accurate measurements to within  $\pm 0.1$  pounds per gallon. The balance is constructed so that the fixed volume cup at one end of the beam is balanced by a fixed counterweight at the opposite end, with a sliding weight rider free to move along the graduated scale. A level bubble mounted on the beam indicates when the system is in balance.

**Specifications:**

8.0 - 25.0 lb / gal  
 960 - 3000 Specific Gravity, kg/meter<sup>3</sup>  
 60 - 189 lb / ft<sup>3</sup>  
 420 - 1300 pounds per inch<sup>2</sup> / 1000 ft

**Calibration:**

OFITE mud balances are calibrated at the factory with the lid included in the mud balance kit. However, the balance should be re-calibrated, if necessary, on site. Any time a mud balance lid, or any other part, is replaced, the instrument should be re-calibrated.

1. The calibration of the instrument may be easily checked by measuring the density of fresh water.
2. Fill the cup with fresh water, and set the rider on the water line at 8.3 pounds per gallon or 1000 kg/m<sup>3</sup>. Add or remove lead shot from the shotwell until the instrument is in balance.

**Procedure:**

1. Place the mud balance base (preferably in carrying case) on a flat level surface.
2. Measure the temperature of the fluid and record on the appropriate mud report form.
3. Fill the clean, dry cup to the top with the freshly obtained mud sample to be weighed.
4. Place the lid on the cup and set it with a gentle twisting motion. Be sure that some mud is expelled through the hole in the cap as this will ensure the cup is full and also will free any trapped air or gas.
5. Cover the hole in the lid with a finger and wash all mud from the outside of the cup and arm. Then thoroughly dry the entire balance.
6. Place the balance on the knife edge and move the rider along the outside of the arm until the cup and arm are balanced as indicated by the bubble.
7. Read mud weight at the edge of the rider toward the mud cup.
8. Clean and dry the mud balance after each use.

**Results:**

Report the mud weight to the nearest 0.1 pound per gallon, 1.0 pound per cubic foot, 10 kilograms per cubic meter, or 10 PSI / 1000 ft.

**Density Conversions:**

Pounds Per Gallon (lb/gal.)	Pounds per Cubic Foot (lb/ft <sup>3</sup> )	Specific Gravity <sup>a</sup> (sg)	Kg per Meter <sup>3</sup> (kg/m <sup>3</sup> )
6.5	48.6	0.78	780
7.0	52.4	0.84	840
7.5	56.1	0.90	900
8.0	59.8	0.96	960
8.3	62.3	1.00	1000
8.5	63.6	1.02	1020
9.0	67.3	1.08	1080
9.5	71.1	1.14	1140
10.0	74.8	1.20	1200
10.5	78.5	1.26	1260
11.0	82.3	1.32	1320
11.5	86.0	1.38	1380
12.0	89.8	1.44	1440
12.5	93.5	1.50	1500
13.0	97.2	1.56	1560
13.5	101.0	1.62	1620
14.0	104.7	1.68	1680
14.5	108.5	1.74	1740
15.0	112.5	1.80	1800
15.5	115.9	1.86	1860
16.0	119.7	1.92	1920
16.5	123.4	1.98	1980
17.0	127.2	2.04	2040
17.5	130.9	2.10	2100
18.0	134.6	2.16	2160
18.5	138.4	2.22	2220
19.0	142.1	2.28	2280
19.5	145.9	2.34	2340
20.0	149.6	2.40	2400
20.5	153.3	2.46	2460
21.0	157.1	2.52	2520
21.5	160.8	2.58	2580
22.0	164.6	2.64	2640
22.5	168.3	2.70	2700
23.0	172.1	2.76	2760
23.5	175.8	2.82	2820
24.0	179.5	2.88	2880

<sup>a</sup>Specific gravity same as Grams per Cubic Centimeter (g/cm<sup>3</sup>)